


5973 Air and Water Check

Instrument: MSD 20

Thu Aug 03 16:05:12 2006

D:\MSDCHEM\1\5973N\ATUNE.U

Scan: 10.00 - 75.00 Samples: 8 Thresh: 0 Step: 0.10
 64 peaks Base: 69.00 Abundance: 570752

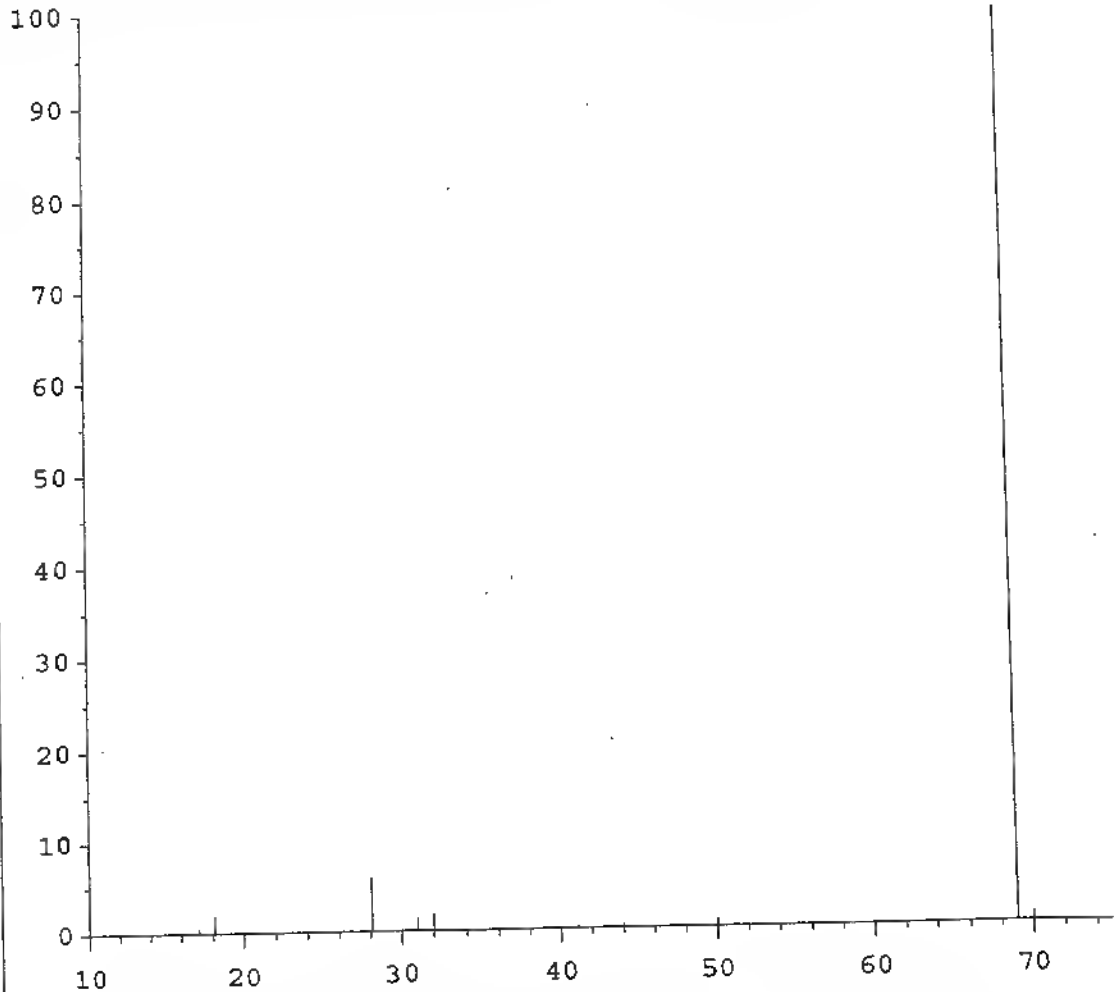

Mass	Abund	Rel Abund	Iso Mass	Iso Abund	Iso Ratio
69.00	570752	100.00	70.00	6224	1.09
18.10	11166	1.96	19.00	68	0.61
28.10	33960	5.95	29.10	901	2.65

Current Params used:

Rep = 30.5 Entl = 19.33 Entr = 12 FOCUS = 90 EMV = 1353

Relative abundances:

18/69 = 1.96	Water%
28/69 = 5.95	Nitrogen%
32/69 = 1.86	Oxygen%
44/69 = 0.40	Carbon Dioxide%
28/18 = 304.14	Nitrogen/Water%